

**AAA DENTALAB**

1st Floor, Unit 4 Watling Gate,
297-303 Edgware Road,
London NW9 6NB.

www.aaadentalab.co.uk

✉ : info@aaadentalab.co.uk

☎ : 0203 6022728

☎ : 07400066241

Impression

Date :

Date

Required:

10 working days required in the lab.

Dentist

Name:

Practice Name :

Postcode (Acc No.):

Patient ID / Code :

☐ Male☐ Female

D.O.B.:

We Accept
All Digital
Scan


☐ NHS ☐ Private / Independent ☐ Implant
Full Metal (Crown / Bridge)

- ☐ Full Cast Non-Precious
☐ Full Cast Semi-Precious
☐ Full Cast Precious 60% (Gold)
☐ Integral Post & Core
☐ Separate Post & Core

Porcelain Fused Metal (PFM)

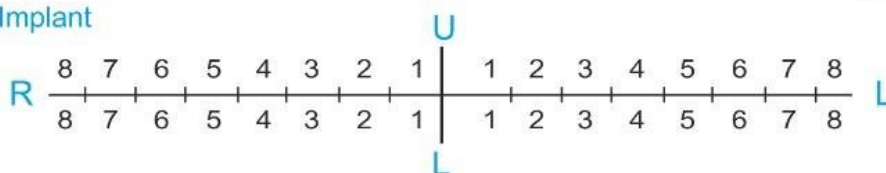
- ☐ PFM Crown Non-Precious
☐ PFM Crown Semi-Precious
☐ PFM Bridge
☐ Maryland Bridge (1 Wing or 2 Wing)

Metal Free Ceramics

- ☐ Composite inlay / Onlay / Crown
☐ Full Zirconia
☐ Zirconia with Emax® Layering
☐ Emax® Inlay/Onlay/Crown/Veneer
☐ Full Zirconia Maryland

Implant

- ☐ Cement Retained
☐ Screw Retained
☐ Custom Abutment(s)
☐ Stock Abutment(s)

**Occlusion**

Tight



0.5mm



1.0mm

Collar and Metal DesignNo
Metal
Collar360°
Metal
CollarMetal
Occlusal
OnlyMetal
Lingual
OnlyMetal
Occlusal
and
LingualMetal
Island**Special Instructions:****Shade**

Vita Classic

If Insufficient Room
☐ Metal Occlusion ☐ Adjust Opposing ☐ Adjust Prep

THIS DEVICE IS NON STERILE *Unless otherwise specified NHS, all work will be processed as private case. (Full Terms & Conditions are attached. or visit our web at www.aaadentalab.co.uk) MHRA No. 8496/GDC No. 285519 / DLA MEMBER

Your attention is drawn to the following statement: This is a custom-made dental device that has been manufactured to satisfy the design characteristics, properties and detail of what has been prescribed by the above dentist. This dental device is purely manufactured for exclusive use of the patient described above. The product meets the general safety and performance requirements specified in the Annex I of Medical Devices Regulations. This product may have been produced in either or both UK and China by AAA Dentalab LTD.

Instructions for use, storing & handling : It is highly recommended that, this dental device is stored in a clean and safe environment that prevents it from coming in contact with materials, liquids or acids that could cause disfiguration or damage to the dental device. The dental device should not be subjected to extreme heat. Where applicable, you should take care not to damage the dental device(s) when removing from its model.

Prescriber Feedback: To enable our dental laboratory to comply with the Medical Devices Regulations for Post Market Surveillance, please inform us of any feedback or issues regarding the enclosed device(s) as soon as possible.